# This Page Is Inserted by IFW Operations and is not a part of the Official Record

### **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- (•) BLACK OR VERY BLACK AND WHITE DARK PHOTOS
  - GRAY SCALE DOCUMENTS

### IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents will not correct images, please do not report the images to the Image Problem Mailbox.

#### Contact Sensitive Device Darius Martin Sullivan and Nicholas P.R. Hill 10/729,540





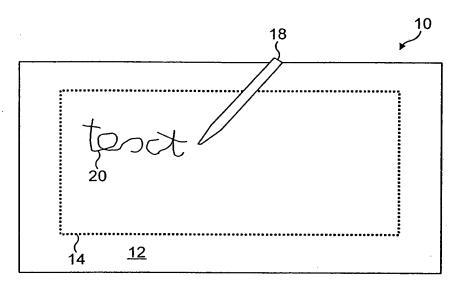


FIG. 1


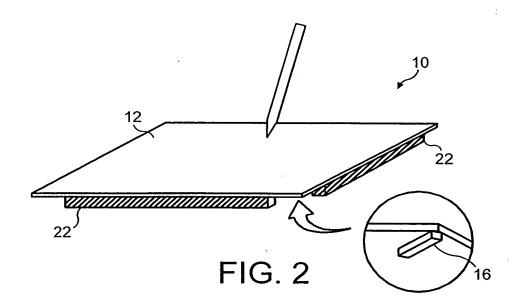




FIG. 3

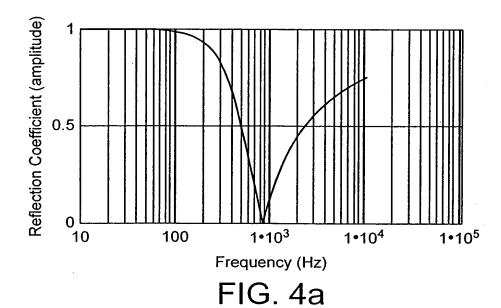

Selection to a selection of the selectio

# Contact Sensitive Device Darius Martin Sullivan and Nicholas P.R. Hill 10/729,540

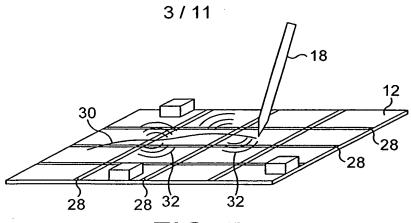


FIG. 5a

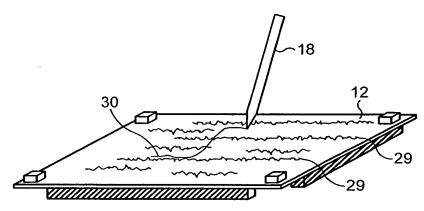


FIG. 5b

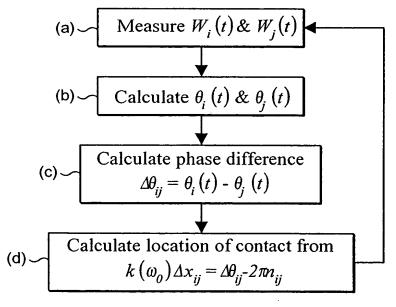


FIG. 6

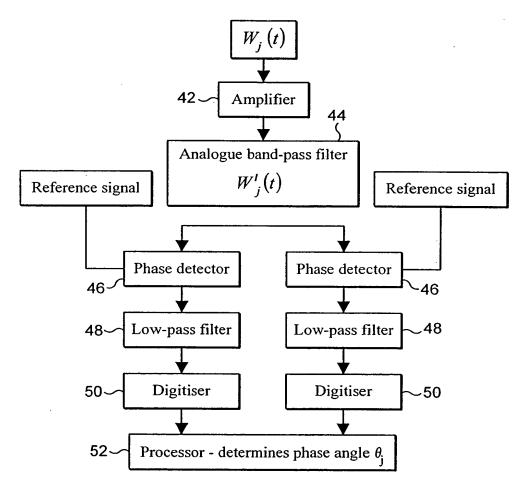


FIG. 7a

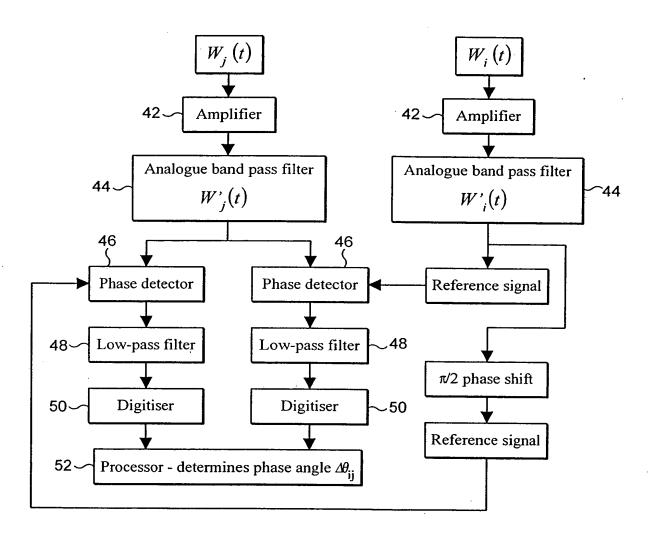


FIG. 7b

6/11




FIG. 8a

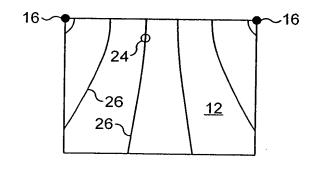


FIG. 8b

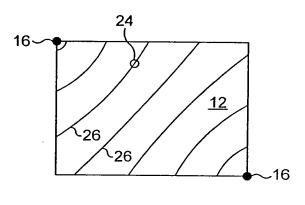


FIG. 8c

. .




FIG. 8d

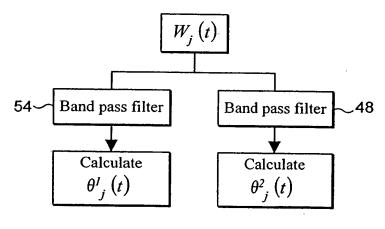


FIG. 9

7/11


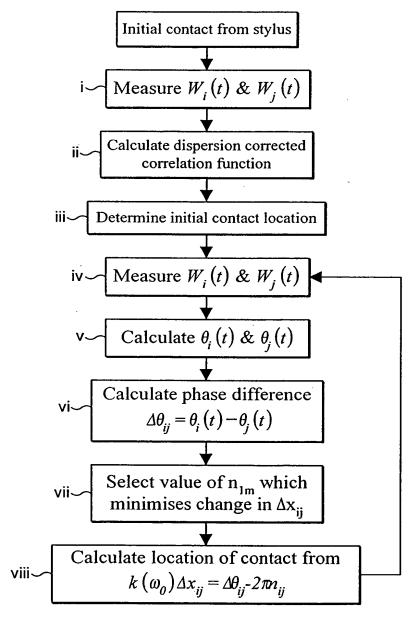


FIG. 10

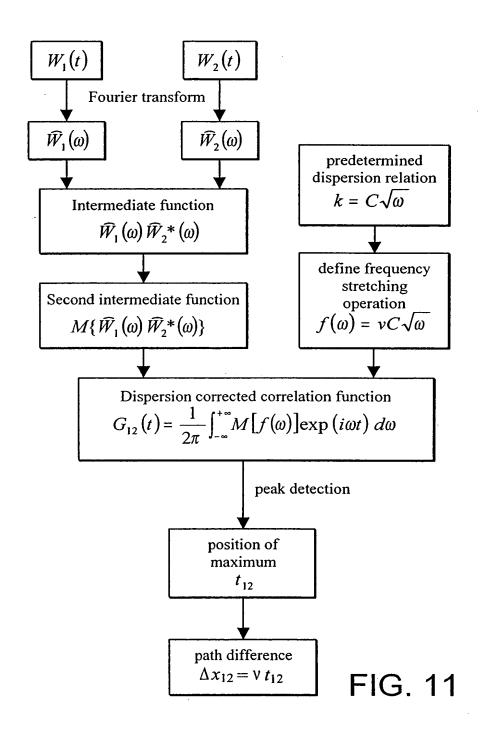

----

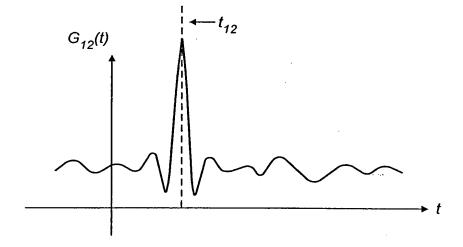


FIG. 11a

. ...

. ....

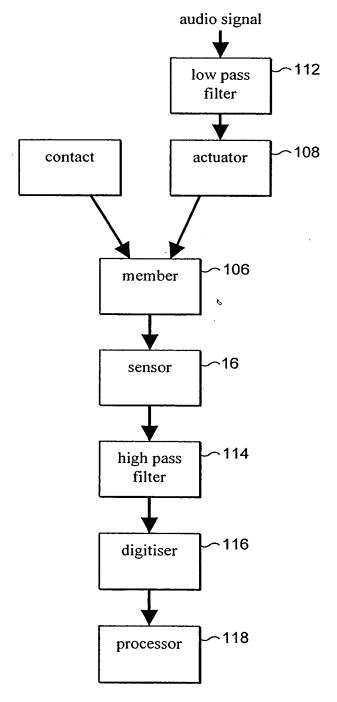


FIG. 12a

